





中国认可 国际互认 检测 TESTING CNAS L0599

Test Report SL52035260669801TX Date:June 18,2020 Page 1 of 4

ZHEJIANG HUAFU MEDICAL EQUIPMENT CO., LTD. NO.688 XINXING 1ST RD., PINGHU, JIAXING, ZHEJIANG PROVINCE, 314200 CHINA

The following sample(s) was/were submitted and identified on behalf of the client as:

Sample Description : (A)Isolation gown

Composition : (A)SMS Sample Color : (A)blue

Manufacturer : ZHEJIANG HUAFU MEDICAL EQUIPMENT CO., LTD.
Supplier : ZHEJIANG HUAFU MEDICAL EQUIPMENT CO., LTD.

Sample Receiving Date : Jun 16, 2020

Testing Period : Jun 16, 2020 - Jun 18, 2020

Test Result(s) : Unless otherwise stated the results shown in this test report refer only to the

sample(s) tested, for further details, please refer to the following page(s).

Test Performed : Selected test(s) as requested by applicant

Signed for and on behalf of SGS-CSTC Standards Technical Services (Shanghai) Co., Ltd Testing Center

Sara Guo (Account Executive)





Test Report

SL52035260669801TX

Date:June 18,2020

Page 2 of 4

Test Result

Liquid Barrier Performance and Classification of Protective Apparel and Drapes Intended for Use in **Health Care Facilities**

(ANSI/AAMI PB70:2012)

Section 4.2.1 Water Resistance: Impact Penetration Test

(AATCC 42-2017)

As received

Weight of blotter gained (g)	1#	2#	3#	4#	5#
Area A (Critical zone-front)	0.0	0.0	0.0	0.0	0.0
Area B (Critical zone-sleeve)	0.0	0.0	0.0	0.0	0.0
Area C (Critical zone-Back)	0.0	0.0	0.0	0.0	0.0
Seam between areas A&B	0.0	0.0	0.0	0.0	0.0
Seam between areas A&C	0.0	0.0	0.0	0.0	0.0
Seam between areas B&C	0.0	0.0	0.0	0.0	0.0

Remark:

- Level 1: all critical zone components shall have a blotter weight gain of no more than 4.5grams(g)
- Level 2: all critical zone components shall have a blotter weight gain of no more than 1.0 grams(g)
- Level 3: all critical zone components shall have a blotter weight gain of no more than 1.0 grams(g)

Section 4.2.1 Water Resistance: Hydrostatic Pressure Test

(AATCC 127-2018; Hydrostatic Head; Rate of increase of water pressure:60mbar/min; temp. of distilled water: 21 ℃, fabric face side of water)

As received

Water Column (cmH ₂ O)	1#	2#	3#	4#	5#
Area A (Critical zone-front)	>50.0	>50.0	>50.0	>50.0	>50.0
Area B (Critical zone-sleeve)	>50.0	>50.0	>50.0	>50.0	>50.0
Area C (Critical zone-Back)	>50.0	>50.0	>50.0	>50.0	>50.0
Seam between areas A&B	>50.0	>50.0	>50.0	>50.0	>50.0
Seam between areas A&C	>50.0	>50.0	>50.0	>50.0	>50.0
Seam between areas B&C	>50.0	>50.0	>50.0	>50.0	>50.0

Remark:

- Level 2: all critical zone components shall have a hydrostatic resistance of at least 20cmH₂O
- Level 3: all critical zone components shall have a hydrostatic resistance of at least 50cmH₂O



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com/en/Terms-and-Conditions/Terms

3rdBuilding,No.889,Yishan Road,Xuhui District Shanghai,China 200233 中国・上海・徐汇区宜山路889号3号楼 邮编: 200233

t (86-21) 61402666

t (86-21) 61402666 f (86-21) 64958763 f (86-21) 64958763 www.sgsgroup.com.cn e sgs.china@sgs.com



Test Report

SL52035260669801TX

Date:June 18,2020

Page 3 of 4

Barrier performance of each component and final classification commended

	Impact Penetration Test AATCC 42(g)	Hydrostatic Pressure Test AATCC 127(cmH2O)	Resistance to Bacteriophage Phi-X174 ASTM F 1671	Level	Final classification
Area A (Critical zone- front)	0.0	>50.0	/	Level 3	Level 3
Area B (Critical zone-sleeve)	0.0	>50.0	/	Level 3	
Area C (Critical zone- Back)	0.0	>50.0	/	Level 3	
Seam between areas A&B	0.0	>50.0	/	Level 3	
Seam between areas A&C	0.0	>50.0	/	Level 3	
Seam between areas B&C	0.0	>50.0	/	Level 3	

Remark:

- The barrier performance of all critical zone components, including seams and points of attachments, shall be determined. The classification of isolation gown shall be a number denoting the performance of the critical zone component having the lower barrier performance.
- Level 1: Impact Penetration Test-AATCC 42: ≤4.5g;
- Level 2: Impact Penetration Test-AATCC 42: ≤1.0g; Hydrostatic Pressure Test-AATCC 127: ≥20cmH₂O;
- Level 3: Impact Penetration Test-AATCC 42: ≤1.0g; Hydrostatic Pressure Test-AATCC 127: ≥50cmH₂O;
- Level 4: Resistance to Bacteriophage Phi-X174-ASTM F 1671: Pass.
- Only test the barrier performance of the sample. Label request, construction and other classed in ANSI/AAMI PB70-2012 is not checked.



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com/en/Terms-and-Conditions/Terms

3rdBuilding,No.889,Yishan Road,Xuhui District Shanghai,China 200233 中国・上海・徐汇区宜山路889号3号楼 邮编: 200233

t (86-21) 61402666

t (86-21) 61402666 f (86-21) 64958763 f (86-21) 64958763 www.sgsgroup.com.cn e sgs.china@sgs.com




Test Report

SL52035260669801TX

Date:June 18,2020

Page 4 of 4

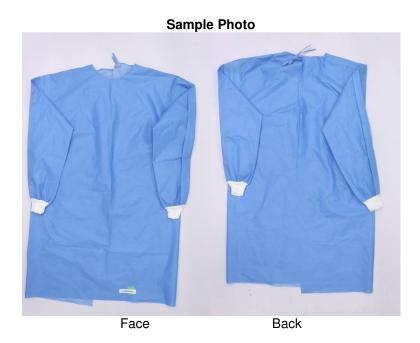

The statement of conformity in this test report is only based on measured values by the laboratory and does not take their uncertainties into consideration.

End of Report



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com/en/Terms-and-Conditions/Terms

3rdBuilding,No.889,Yishan Road,Xuhui District Shanghai,China 200233 中国・上海・徐江区宜山路889号3号楼 邮编: 200233 t (86-21) 61402666 t (86-21) 61402666 f (86–21) 64958763 f (86–21) 64958763 www.sgsgroup.com.cn e sgs.china@sgs.com